

## DEVELOPMENT OF A HARDWARE MODULES FOR THE PRIMARY DIAGNOSIS OF GASTROINTESTINAL DISEASES

Yakhshiboyev R. E.

Tashkent University of Information Technologies named after Muhammad al-  
Khwarizmi Tashkent, Uzbekistan  
[yaxshiboyevrustam@gmail.com](mailto:yaxshiboyevrustam@gmail.com)

### Abstract

The article deals with the issues of diagnosing gastrointestinal diseases based on human saliva. The results obtained in solving the problems of identifying and primary diagnosis of gastrointestinal symptoms as a result of a change in the composition of saliva were analyzed and the results obtained were compared with the results obtained in the works of other scientists.

**Keywords**— Saliva device, sensor, ADC, UART, LM2596 controller, Bluetooth

### I.INTRODUCTION

Currently, many modern solutions have been developed to detect diseases in human saliva at any time of daily activities. In each of the proposed solutions, the hardware and software of devices is used to detect symptoms of various types of diseases, diagnose or remotely monitor certain diseases [1,2,3].

This article presents an analysis of the 7-channel hardware-software complex "Saliva" for the primary diagnosis of gastroenterological diseases.

This hardware and software complex, designed for the population living outside medical institutions or hard-to-reach areas, was developed in accordance with the following requirements:

Availability of equipment and software for primary diagnostics;

The device can be used at home and by gastroenterologists for daily activities;

Cheap enough for everyone;

Long-term operation of the power supply;

## II. DEVELOPMENT OF HARDWARE-SOFTWARE COMPLEX MODULES

Devices for the primary diagnosis of diseases of the gastrointestinal tract is called "Saliva". The device consists of sensor, ADC, microcontroller, UART, Regulator and Bluetooth. When developing the Saliva device, special attention was paid to its low cost and ease of carrying [9,10,11].

The architecture of the "Saliva" system consists of functional blocks and each performs certain tasks, Figure - 1.1. The "Saliva" system consists of 5 main modules, and they make up the hardware-software complex.

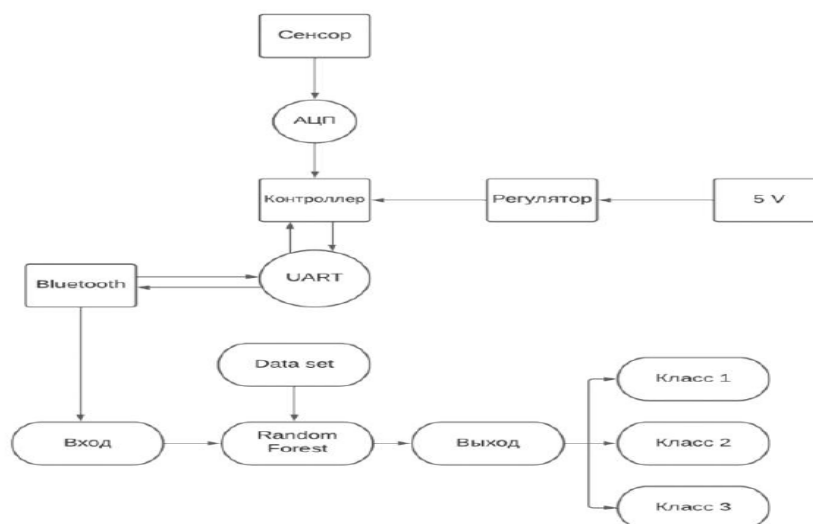


Fig 1.1. Functional module of the "Saliva" device

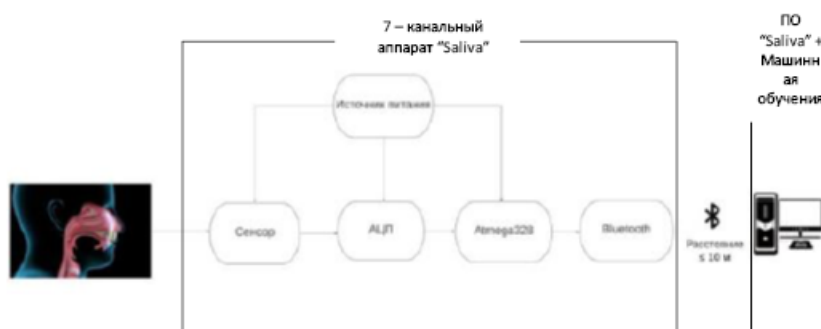


Fig 1.2. Structure of the 7-channel hardware-software complex "Saliva"

Figure 1.2 shows the structure of the 7-channel hardware-software complex “Saliva”, which consists of 5 main modules, together with them it makes up the hardware-software complex of the device [12,13,14].

Based on the structural image of the Saliva hardware-software complex, we can distinguish the main modules as:

**Sensors** - according to the selected parameters, it makes up a set of sensors for protein, glucose, mucin, cholesterol, ammonium and uric acid. Here, the sensor performs the task of both obtaining a substance for analysis and a recognizer for subsequent processes. Since, using the example of human saliva, we know about its content of substances and enzymes [15,16,17].

An analog-to-digital converter (ADC) is a device that converts an input analog signal into a discrete code, that is, converts it into a digital one. In the ADC chip, all channels are discredited simultaneously. The gain parameters of the ADC chip can be adjusted by the PGA.

**PGA at a Glance** - Digital Programmable Gain Instrumentation Operational Amplifiers (PGAs) are versatile input op-amps that digitally control gain to improve accuracy and increase dynamic range.

After the sensor determines all the constituent components of saliva as an analog object, the information is transmitted precisely to the ADC, as mentioned above. The ADC converts the information received from the sensor into a binary code. This chip allows you to measure the patient's saliva according to the selected parameters, can use the RLD scheme, the data transmission of the chip can reach a speed of 500-32 kbps (the value of the transmitted discrete frequency is 103 seconds). The connection between the “Saliva” device and the computer is established through the UART interface [16,17,18].

**Atmega328 microcontroller.** ATmega328 microcontroller is 8-bit CMOS low power microcontroller based on advanced AVR RISC architecture. The microcontroller receives the primary processed signal of the saliva sample coming from

ADS1298 chips in the power supply of the “Saliva” device and performs secondary processing and transfers them to the Bluetooth module via the SPI interface. The microcontroller also controls the ADC module, a 7-channel device for a discrete and



analog-to-digital saliva sample signal converter and other peripheral devices. Communication between the Atmega328 and peripherals was implemented using the SPI module. Block diagram of the Atmega328 microcontroller [1,2,3].

The Atmega328 microcontroller is connected to two SPI interfaces that support high-speed data exchange with ADC and Bluetooth NS-05 devices. The ADC module provides a serial communication clock system. Synchronization in all communication processes should be at least minimal.

Bluetooth HC-05. Bluetooth HC-05, one of the main power modules of the “Saliva” device, provides the process of wireless data exchange between the computer and the “Saliva” device via the UART interface. The frequency range of the HC-05 module and the data transmission channel correspond to ISM, i.e. 2.4 GHz. This intermediate frequency is the radio frequency range defined by the radio regulations of the International Telecommunication Union [4,5,6].

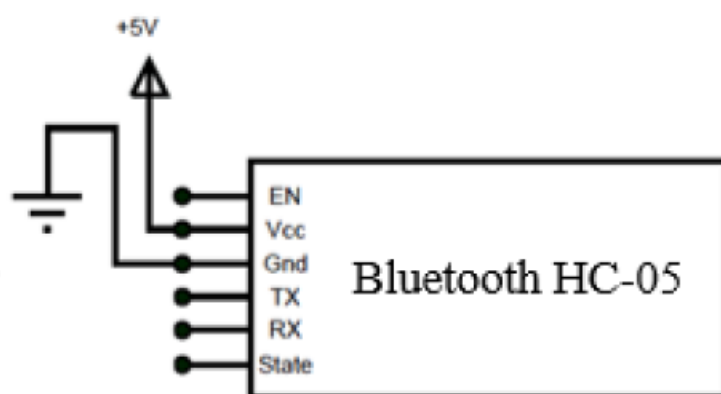


Figure 1.4. Block diagram of Bluetooth module HC-05

The total size of information of 8 channels coming from the ADS1298 device is  $224 \times 8 = 224 \times 23 = 227$ , that is,  $227 \times 50/8 = 838\ 860\ 800$  or  $838\ 860\ 800/1024 = 819\ 200$  Kbps or 800 Mb.

If this value is expressed in the 16th number system, it will be equal to  $800/216 = 0.0122$  MB. The total bandwidth of the Bluetooth NS05 device selected for designing the ECG device is 2.1 Mbps, which is about 10 times more than the digital data (0.0122 Mbps) generated by the ADC device, which is in line with the current demand.

Bluetooth HC-05 has two different states (modes): command state and transmit/receive state. 38400kbps in command mode and 9600kbps in data transmission/reception mode.



Fig 1.3. Atmega328 microcontroller.

### III. CONCLUSION

As a result, we can say that with the help of this developed hardware-software complex, it is possible to reduce the time of diagnosis. The hardware-software complex can be further used in polyclinics and as an auxiliary complex for a gastroenterologist. The hardware and software complex were developed jointly with the 2-clinic of the Tashkent Medical Academy, with gastroenterologists.

### REFERENCES

- [1] Neishaboori A, Moshrefiaraghi D, Mohamed Ali K, Toloui A, Yousefifard M, Hosseini M. Central Nervous System Complications in COVID-19 Patients; a Systematic Review and Meta-Analysis based on Current Evidence. Arch Acad Emerg Med. 2020
- [2] Koralnik IJ, Tyler KL. COVID-19: A Global Threat to the Nervous System. Ann Neurol. 2020;88(1):1-11. doi:10.1002/ana.25807
- [3] Asadi-Pooya AA, Simani L. Central nervous system manifestations of COVID-19: A systematic review. J Neurol Sci. 2020; 413:116832. doi:10.1016/j.jns.2020.116832

[4] Lu N, Xing DQ, Sheng T, Lu W. Sheng Li Xue Bao. The mechanism and function of hippocampal neural oscillation. Acta Physiologica Sinica, October 25, 2017, 69(5): 647–656 DOI: 10.13294/j.aps.2017.0052 <http://www.actaps.com.cn>

[5] B. N. Hidirov, Izbrannye raboty po matematicheskomu modelirovaniyu reguljatoriki živyh sistem. Moskva – Iževsk, 2014, 304 s.

[6] Saidalieva M., Hidirova M. Quantitative analysis of the regulatory mechanisms of living systems to identify effective influence points during anomalies // International Conference on Information Science and Communications Technologies ICISCT 2019. 4-6 November 2019. Tashkent. pp. 1-3.

[7] Khamzaev J. et al. DRIVER SLEEPINESS DETECTION USING CONVOLUTION NEURAL NETWORK //CENTRAL ASIAN JOURNAL OF EDUCATION AND COMPUTER SCIENCES (CAJECS). – 2022. – Т. 1. – №. 4. – С. 31-35.

[8] Яхшибоев Р. и др. РАЗРАБОТКА МОДЕЛИ РАСПОЗНАВАНИЯ ГРАФИЧЕСКИХ ОБЪЕКТОВ НА ОСНОВЕ МЕТОДА «TRANSFER LEARNING» ДЛЯ ДИАГНОСТИКИ В СФЕРЕ ЗДРАВООХРАНЕНИЯ //Conferences. – 2022. – С. 156-164.

[9] Yaxshiboyev R. DEVELOPMENT OF A SOFTWARE AND HARDWARE COMPLEX FOR PRIMARY DIAGNOSTICS BASED ON DEEP MACHINE LEARNING //CENTRAL ASIAN JOURNAL OF EDUCATION AND COMPUTER SCIENCES (CAJECS). – 2022. – Т. 1. – №. 4. – С. 20-24.

[10] Яхшибоев Р., Базарбаев М., Эрметов Э. ПРИМЕНЕНИЕ НЕЙРОННЫХ СЕТЕЙ ДЛЯ ДИАГНОСТИКИ МЕДИЦИНСКИХ ЗАБОЛЕВАНИЙ //Conferences. – 2022. – С. 148-156.

[11] Yaxshiboyev R. DEVELOPMENT OF A MODEL OF OBJECT RECOGNITION IN IMAGES BASED ON THE «TRANSFER LEARNING» METHOD //CENTRAL ASIAN JOURNAL OF EDUCATION AND COMPUTER SCIENCES (CAJECS). – 2022. – Т. 1. – №. 4. – С. 36-41.

[12] Яхшибоев Р. Э., Очилов Т. Д., Сиддиков Б. Н. РАЗРАБОТКА ПРОГРАММНОГО СРЕДСТВА ДЛЯ ИДЕНТИФИКАЦИИ НОМЕРНЫХ ЗНАКОВ ТРАНСПОРТНЫХ СРЕДСТВ НА ОСНОВЕ МЕТОДОВ





КОМПЬЮТЕРНОГО ЗРЕНИЯ //Journal of new century innovations. – 2022. – Т. 15. – №. 1. – С. 81-93.

[13] Яхшибоев Р., Сиддиков Б. ЦИФРОВЫЕ ТЕХНОЛОГИИ ДЛЯ ПЕРВИЧНОЙ ДИАГНОСТИКИ РАЗНЫХ МЕДИЦИНСКИХ ЗАБОЛЕВАНИЙ //Innovations in Technology and Science Education. – 2022. – Т. 1. – №. 4. – С. 94-105.

[14] Yaxshiboyev R., Yaxshiboyeva D. ANALYSIS OF ALGORITHMS FOR PREDICTION AND PRELIMINARY DIAGNOSTICS OF GASTROENTEROLOGICAL DISEASES //CENTRAL ASIAN JOURNAL OF EDUCATION AND COMPUTER SCIENCES (CAJECS). – 2022. – Т. 1. – №. 2. – С. 49-56.

[15] Djumanov J. et al. Mathematical model and software package for calculating the balance of information flow //2021 International Conference on Information Science and Communications Technologies (ICISCT). – IEEE, 2021. – С. 1-6.

[16] Yaxshiboyev R. E. et al. FORECASTING GROUNDWATER EVAPORATION USING MULTIPLE LINEAR REGRESSION //Galaxy International Interdisciplinary Research Journal. – 2021. – Т. 9. – №. 12. – С. 1101-1107.

[17] Кудратиллаев М.Б. ПРОМЫШЛЕННЫЙ ИНТЕРНЕТ ВЕЩЕЙ (IIoT), КАК НОВАЯ ТЕХНОЛОГИЯ В СФЕРЕ ПРОИЗВОДСТВЕННОЙ ИНДУСТРИИ // "Prospects for the development of the electric power sector in the south of the republic" International conference.-2022.-С.381-386.

[18] Pulatov Sh.U., Kudratillaev M. PROSPECTS FOR THE DEVELOPMENT OF FIFTH- GENERATION NETWORKS (5G) IN UZBEKISTAN // 2022 International conference "Recent advances in intelligent information and communication technology". – TUIT,2022.-С. 393-397.

